



Correlate-Enzyme™ Assay

Chemiluminescent Cyclooxygenase Activity Kit

Catalog No. 907-011

100 Test Tube (12 x 75 mm) Kit

Table of Contents

Description	Page	2
Introduction		2
Precautions		3
Materials Supplied		3
Storage		3
Materials Needed but Not Supplied		3
Sample Handling		4
Procedural Notes		4
Typical Inhibition Assay		5
Luminescent Assay Procedure		6
Calculation of Results		7
Typical Results		7
Typical Standard Curves		8
Performance Characteristics		9
Interfering Substances		10
Sample Dilution Recommendations		11
References		11
Limited Warranty		12

Simplify Your Science®

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.


Description

Assay Designs' Correlate-Enzyme™ Chemiluminescent Cyclooxygenase Activity kit is for the quantitative determination of Cyclooxygenase activity in biological samples. Please read the complete kit insert before performing this assay.

Introduction

Cyclooxygenase (COX, also known as Prostaglandin G/H synthase) is a membrane bound enzyme responsible for the oxidation of arachidonic acid to Prostaglandin G₂ (PGG₂) and the subsequent reduction of PGG₂ to PGH₂^{1,2}. The conversion is shown below. These reactions are the first steps in the formation of a variety of prostanoids. COX has been shown to be expressed in at least two different isoforms: a constitutively expressed form, COX-I, and an inducible form, COX-II. COX-I is thought to regulate a number of 'housekeeping' functions, such as vascular hemostasis, renal blood flow, and maintenance of glomerular function³. Inflammation mediators such as growth factors, cytokines and endotoxin induce COX-II expression in a number of cellular systems^{4,5}. The effect of various non-steroidal anti-inflammatory drugs (NSAIDs) on the activity of COX-I and -II is an area of considerable interest. Some methods to determine COX activity involve procedures such as measuring uptake of oxygen using an oxygraph, measuring the conversion of radioactive arachidonic acid, or measuring the prostaglandins formed from PGH₂ (such as determining PGE₂ using immunoassays⁶)+Q Most of these methods are complex, time consuming, and are prone to interferences.

The Cyclooxygenase Reaction

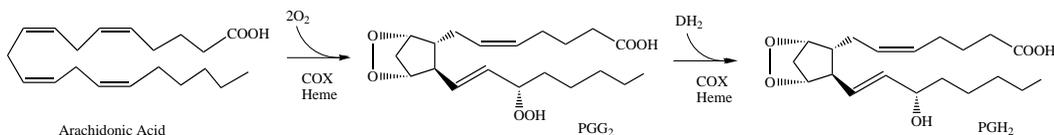

Assay Designs' Cyclooxygenase Activity Kit uses a specific chemiluminescent substrate to detect the peroxidative activity of COX enzymes. After inhibition by NSAIDs, the direct residual activity of COX is measured by addition of a proprietary luminescent substrate and arachidonic acid. Light emission starts immediately and is directly proportional to the COX activity in the sample. The chemiluminescent signal is measured over 5 seconds.

Note: In this insert, one Unit of COX activity is defined as the amount of enzyme needed to consume 1 nmole of oxygen per minute at 37 °C.

Precautions

FOR RESEARCH ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

1. The luminescent substrate is an aromatic hydrocarbon molecule with unknown biological effects. Care should be used in handling this reagent.
2. The test tubes supplied in this kit have been selected for their low luminescent background and excellent reproducibility. Some glass and plastic tubes, especially soda lime glass tubes, exhibit highly variable phosphorescence that will interfere with the assay.
3. The NSAIDs supplied in the kit, Catalog Nos. 80-0276 and 80-1345, have known and unknown effects on biological tissue. Care should be taken in handling these materials.

Materials Supplied

1. **Polypropylene test tubes, 12 x 75mm, 100 tubes, Catalog No. 80-0274**
Polypropylene test tubes selected for low background luminescence and reproducible light measurement.
2. **COX Chemiluminescent Substrate, 10 mL, Catalog No. 80-0275**
A solution of chemiluminescent substrate in aqueous buffer. **Substrate is sensitive to light.** Protect solution from ambient room light.
3. **Ibuprofen, 2 mL, Catalog No. 80-0276**
A 300 mM solution of ibuprofen (α -Methyl-4-(isobutyl)phenylacetic acid) in water.
4. **Meloxicam, 2 mL, Catalog No. 80-1345**
A 1mM solution of Meloxicam (CAS No. 71125-38-7) in DMSO.

Storage

All components of this kit, **except the Ibuprofen and Meloxicam**, are stable at 4 °C until the kit's expiration date. The Ibuprofen and Meloxicam **must** be stored at or below -20 °C.

Materials Needed but Not Supplied

1. Deionized or distilled water.
2. Precision pipets for volumes between 25 μ L and 1,000 μ L.
3. Repeater pipets for dispensing 50 μ L.
4. Disposable beakers and graduated cylinders.
5. Tube luminometer. Instruments that are capable of measuring multiple samples must be equipped with dual injectors for optimal results.
6. COX Inhibition Assay. This kit does not contain materials needed for an inhibition assay (cyclooxygenase, arachidonic acid, or hematin). These must be obtained from other sources. On page 5 we outline a typical inhibition assay protocol. These conditions have been used for the Quality Control testing of this detection kit. It is important that the end user optimize their inhibition assays in line with published studies⁶⁻⁹.

Sample Handling

Assay Designs' Cyclooxygenase Activity Kit is compatible with samples in a wide range of matrices. The procedure described in the Typical Inhibition Assay section is for reference only and the end user must independently determine the proper format and matrix for their inhibition studies. We have tested this assay in a number of buffer systems, but the end user will have to obtain information about compatibility of the assay to measure cyclooxygenase activity in some samples, especially those from tissue sources.

We recommend that at least 10 Units/mL (i.e., approximately 0.5 Units per tube) of either COX-I or COX-II are used for NSAID inhibitor studies. Even though this assay will allow accurate measurements of COX activity down to less than 5 Units/mL, for accurate inhibitor calculations we recommend using higher levels of enzyme.

Procedural Notes

1. Do not mix reagents from different lot numbers or use reagents beyond expiration date.
2. Allow all reagents to warm to room temperature for at least 30 minutes before opening.
3. Pre-rinse the pipet tip with reagent, use fresh pipet tips for each sample, standard and reagent.
4. Add the reagents to the side of the tube to avoid contamination.
5. Mix the substrate well prior to use.
6. **This assay uses a luminescent measurement of COX activity. The luminescent signal is typically represented as Relative Light Units (RLU). Different luminometers will display different RLU readings. Please see the luminometer Instruction Manual for details.**
7. **In this insert one Unit of COX activity is defined as the amount of enzyme needed to consume 1 nmole of oxygen per minute at 37 °C.**

Typical Inhibition Assay

Preparation Protocol

- (1) Store COX-I and/or COX-II at -70 °C or lower. Enzyme dilutions in 100 mM phosphate, pH 7.5, used for inhibition reactions, must be kept at 0-4 °C in an ice bath. These enzyme dilutions are stable for 2-8 hours.
- (2) Prepare hematin (Sigma H-3281, porcine) by dissolving in DMSO at 0.380 mg/mL. The concentrated stock can be stored at -80 °C in single use volumes. Dilute in 100 mM phosphate, pH 7.5 to a final concentration of 0.12 µM. Diluted hematin is stable for up to 8 hours at room temperature.

Avoid exposure to light.

Higher concentrations of hematin give rise to increasing background signals and do not result in increased cyclooxygenase activity or increased inhibition by NSAIDs.

- (3) Prepare a 100 mM Tris, 0.5mM phenol buffer, pH 7.3. Buffer pH must be measured at 37 °C for correct pH measurement.
- (4) Arachidonic acid stock solution in ethanol is prepared by taking a freshly opened vial of arachidonic acid and adding ethanol under argon or nitrogen gas to give a 50 mg/mL solution. Store in the dark at -70 °C or lower.
- (5) Activation of arachadonic acid is carried out by the following procedure. Add 94 µL of 0.1N sodium hydroxide to a glass vial. Add 6 µL of the ethanolic arachadonic acid solution to the vial. Vortex. Dilute the mixture with 9.9 mL of deionized water. Store the prepared solution of arachidonic acid at 0-4 °C in an ice bath; it is stable for up to 3 hours.

For best reproducibility we recommend storing the prepared arachadonic acid solution at 0-4 °C in the luminometer. Injection of the cold arachadonic acid solution is recommended.

Luminescent Assay Procedure

All samples should be run in duplicate.

All samples should be allowed to warm to room temperature and all activity measurements should be run at room temperature.

Assay Protocol

1. Pipet 50 μL of the Tris-phenol buffer into all tubes.
2. Add 50 μL of the hematin solution into all tubes.
3. Add 50 μL COX-I or COX-II preparations to all tubes, except for the Blank and Zero Activity tubes.
4. Pre-incubate at room temperature for 5 minutes.
5. Add 25 μL of NSAID inhibitor solution to appropriate tubes.
6. Incubate at room temperature for 5-120 minutes (dependent on inhibitor).
7. Place polypropylene tubes in luminometer for the chemiluminescent measurement.
8. Inject 50 μL of **cold** COX Chemiluminescent Substrate.
9. Immediately inject 50 μL of diluted **cold** arachidonic acid solution.
10. Immediately read in a luminometer for 5 seconds. Determine integrated light output for the 5 second read time in Relative Light Units (RLU).

If your luminometer has automated injection capabilities, program the instrument to carry out steps 8-10 with minimum delay between steps 8 and 9, and with zero delay between step 9 and light detection.

We have supplied solutions of the COX inhibitors Ibuprofen and Meloxicam to allow users of this kit to distinguish between COX-I and COX-II activity in some samples. Meloxicam is a specific inhibitor of COX-II. Ibuprofen is a non-selective inhibitor of both COX-I and -II.

Calculation of Results

Several options are available for the calculation of the inhibition of cyclooxygenase in the samples. We recommend that the data be handled by an software package utilizing a curve fitting program. If data reduction software is not readily available the data can be transformed as follows:

1. Calculate the average net Relative Light Units (RLU) for each standard and sample by subtracting the average blank RLU from the average RLU for the standards and samples:

$$\text{Average Net RLU} = \text{Average RLU} - \text{Average Blank RLU}$$

2. Percent inhibition should be calculated using the following formula for each inhibitor:

$$\text{Percent Inhibition} = \left(1 - \frac{\text{Average Net Inhibitor RLU}}{\text{Average Net RLU for non-inhibited Enzyme}} \right) \times 100$$

Typical Results

The results shown below are for illustration only and **should not** be used to calculate results from another assay.


Sample	<u>Cyclooxygenase-I</u>			<u>Cyclooxygenase-II</u>		
	<u>COX-I</u> (Units/mL)	<u>Net RLU</u>	<u>Percent Inhibition</u>	<u>COX-II</u> (Units/mL)	<u>Net RLU</u>	<u>Percent Inhibition</u>
S0	0	311		0	655	
S1	60	15,691		60	25,442	
S2	30	2,603		30	15,075	
S3	15	812		15	2,531	
S4	7.5	429		7.5	1,835	
Ibuprofen	60	1,748	88.9%*	60	2,451	90.4%*
Meloxicam	60	7,246	53.8%*	60	10,070	60.4%*

***Actual level of inhibition seen will be dependent on assay conditions used.**


Typical Standard Curves

Typical standard curves are shown below. The concentrations of COX-I and COX-II were varied from 0 to 60 Units/mL and run as described in Step 1 of the Typical Inhibition Assay on page 5. These curves **must not** be used to calculate COX concentrations; each user must run a standard curve for each assay.

COX-I Standard Curve

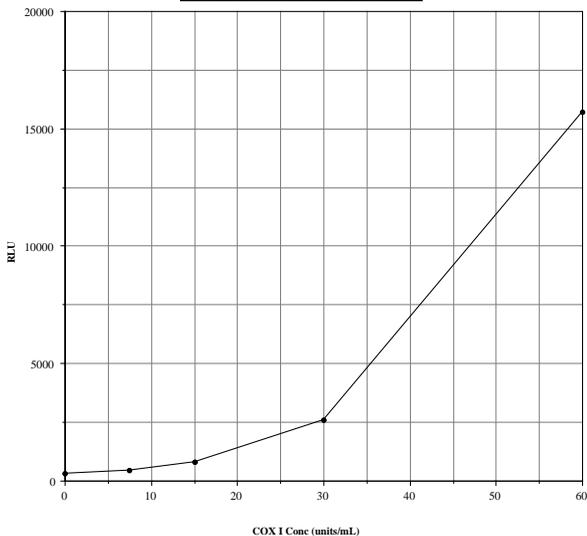

COX-II Standard Curve

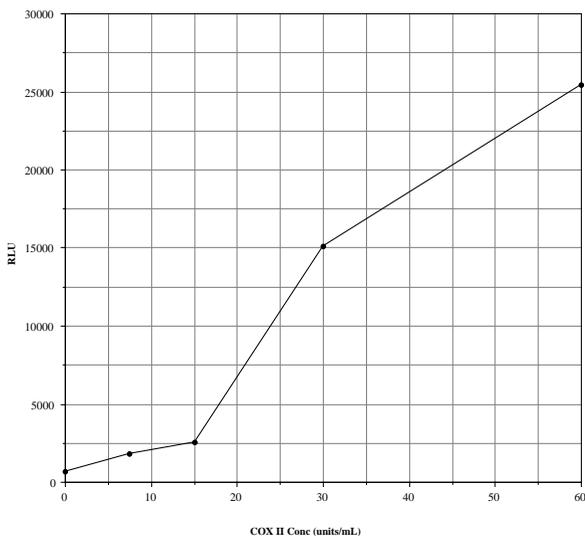


Typical Kinetic Output

A typical kinetic profile of the light emission is also shown to the right.

Performance Characteristics

The following parameters for this kit were determined in the plate format, Catalog No. 907-003, using the guidelines listed in the National Committee for Clinical Laboratory Standards (NCCLS) Evaluation Protocols¹⁰.

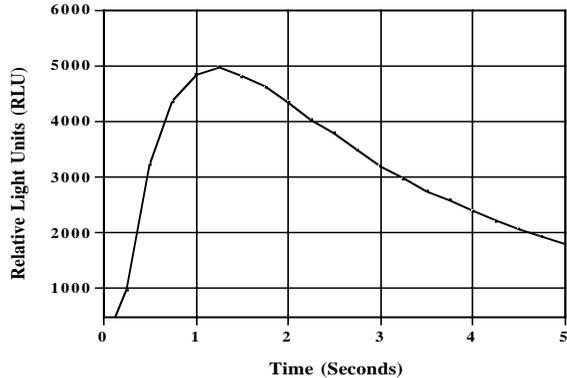

Sensitivity

Sensitivity was calculated by determining the average RLUs for sixteen (16) wells run with 0 Units/mL, and comparing to the average RLUs for sixteen (16) wells run with Standard #4. The detection limit was determined as the concentration of COX-I measured at two (2) standard deviations from the 0 Units/mL Standard along the standard curve.

$$\text{Average RLU for } S_0 = 942 \pm 95 (10.1\%)$$

$$\text{Average RLU for Standard \#4} = 10,667 \pm 544 (5.1\%)$$

$$\text{Delta RLU's (7.5-0 Units/mL)} = 9,725$$

$$2 \text{ SD's of 0 Units/mL Standard} = 190$$

$$\text{Sensitivity} = \frac{190}{9,725} \times 7.5 \text{ Units/mL} = 0.147 \text{ Units/mL COX-I}$$

Using a 50 µL sample, 0.00732 Units of COX-I activity can be detected (corresponds to 7.32 mUnits of COX activity using 1 Unit = 1 nmole of oxygen consumed at 37 °C. See # 7 on page 4.)


Precision

Intra-assay precision was determined by taking samples containing low and high concentrations of COX-I and running these samples multiple times (n=16) in the same assay. The precision numbers listed below represent the percent coefficient of variation for the concentrations of COX-I determined in these assays as calculated by a 4 parameter logistic curve fitting program.

	<u>COX-I Concentration (Units/mL)</u>	<u>RLU's</u>	<u>RLU Intra-assay (%CV)</u>
High	30	78,972	7.0
Low	7.5	19,193	3.1

Effect of Arachidonic Acid

The following graph shows the effect of varying arachidonic acid concentration on light emission. In this example 2 Units of COX-I were used per well. Note that any change in arachidonic acid concentration above 25 μM has very little effect on light output.

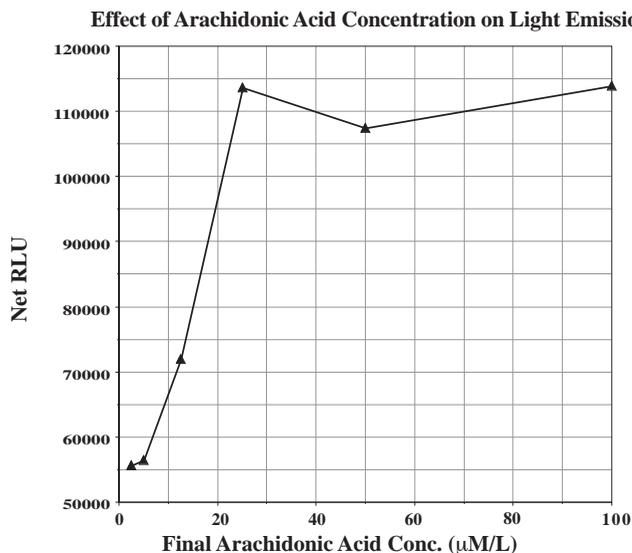

Interfering Substances

The following commonly used substances were tested for interference with the luminescent signal generated in the Cyclooxygenase Activity Kit. At the concentrations listed, the following change in luminescent signal generation was observed.

<u>Substance</u>	<u>Tested Conc.</u>	<u>Signal Change (%)</u>
Ethanol	5%	6
Methanol	5%	1
Dimethyl sulfoxide (DMSO)	10%	1
N,N-Dimethyl formamide (DMF)	1%	12.7
Tween 20	0.1%	5
EDTA	2.5mM	7.3
Protein	0.1%	0
Protease Inhibitors*	0.1%	3.3
Tissue Culture Media	100%	14.8
PBS	100%	15.9
Sodium Azide	0.1%	5.5
Gentamicin	0.01%	0.1

*Contains Peafabloc, pepstatin, leupeptin, E-64, bestatin & aprotinin

References

1. J.R. Vane and R.M. Botting, Inflamm. Res., (1995) 44: 1-10.
2. W.L. Smith, et al., “Intracellular Messengers”, (1993) London: Pergamon Press. 101-136.
3. P. Mene, et al., Physiol. Rev., (1989) 69: 1347-1423.
4. H. Herschman, et al., J. Lipid. Med., (1993) 6: 89-99.
5. E.A. Meade, et al., J. Lipid. Med., (1993) 6: 119-129.
6. S. Kargman, et al., Biochem. Pharm., (1996) 52: 1113-1125.
7. T. Klein, et al., Biochem. Pharm., (1994) 48: 1605-1610.
8. J.K. Gierse, et al., J. Biol. Chem., (1996) 271: 15810-15814.
9. C.M. Markey, et al., J. Biol Chem., (1987) 262: 6266-6279.
10. National Committee for Clinical Laboratory Standards Evaluation Protocols, SC1, (1989) Villanova, PA: NCCLS.

LIMITED WARRANTY

Assay Designs, Inc. warrants that at the time of shipment this product is free from defects in materials and workmanship. This warranty is in lieu of any other warranty expressed or implied, including but not limited to, any implied warranty of merchantability or fitness for a particular purpose.

Assay Designs must be notified of any breach of this warranty within 48 hours of receipt of the product. No claim shall be honored if Assay Designs is not notified within this time period, or if the product has been stored in any way other than outlined in this publication. The sole and exclusive remedy of the customer for any liability based upon this warranty is limited to the replacement of the product, or refund of the invoice price of the goods.




For more details concerning the information within this kit insert, or to order any of Assay Designs' products, please call (734) 668-6113 between 8:30 a.m. and 5.30 p.m. EST. Orders or technical questions can also be transmitted by fax or e-mail 24 hours a day.

Material Safety Data Sheet (MSDS) available on our website or by fax.

**Assay Designs, Inc.
800 Technology Drive
Ann Arbor, MI 48108
U.S.A.**

**Telephone: (734) 668-6113
(800) 833-8651 (USA & Canada only)
Fax: (734) 668-2793
e-mail: info@assaydesigns.com
web: www.assaydesigns.com**

**Methods
for
Molecules™**



Catalog No. 25-0096

March 9, 2005

© 2000

